

3430 Schmon Parkway Thorold, ON, Canada L2V 4Y6 Phone: 866-667-4362 • (905) 227-8848

Fax: (905) 227-1061 Email: techsupport@norgenbiotek.com

# Xylella fastidiosa TaqMan PCR Kit Product# TM67050

### **Product Insert**

#### **Intended Use**

Norgen's *Xylella fastidiosa* TaqMan PCR Kit is designed for the detection of *Xylella fastidiosa* specific DNA in a real-time PCR based on the use of TaqMan® technology. This kit is designed for research use only and not for use in diagnostic procedures.

#### **Background Information**

Xylella fastidiosa is an Gram-negative bacteria and is transmitted by xylem fluid feeding sap insects. Diseases related with X. fastidiosa are bacterial leaf scorch, oleander leaf scorch, coffee leaf scorch (CLS), alfalfa dwarf, phony peach disease, and the economically important Pierce's disease of grapes (PD), citrus variegated chlorosis (CVC) and olive quick decline syndrome (OQDS) in Europe. X. fastidiosa is currently regulated in the EU as a quarantine organism. Pathogenicity of the bacterium only occurs when a large proportion of xylem vessels in a plant are colonized thus many plants are asymptomatic carriers of X. fastidiosa, which can contribute to its spread. Early and sensitive detection could prevent the spreading and help effective pest control.

### **Product Description**

Norgen's *Xylella fastidiosa* TaqMan PCR Kit is designed for the detection of *Xylella fastidiosa* specific DNA in a real-time PCR based on the use of TaqMan technology. This kit is designed for research use only and not for use in diagnostic procedures. The detection of *Xylella fastidiosa* specific DNA is based on TaqMan PCR providing a simple, reliable and rapid result for the detection of *Xylella fastidiosa* infection. Norgen's *Xylella fastidiosa* TaqMan PCR Kit includes a PCR control to monitor for PCR inhibition, and to validate the quality of the sample and the detection result. The *Xylella fastidiosa* TaqMan PCR Kit comprises Master Mix for the target and PCR control detection, Primer & Probe Mix, as well as a positive control and a negative control (nuclease-free water) to confirm the integrity of the kit reagents.

Norgen's *Xylella fastidiosa* TaqMan PCR Kit was developed and validated to be used with the following PCR instruments:

- · Qiagen Rotor-Gene Q
- BioRad CFX96 Touch™ Real-Time PCR Detection System
- QuantStudio<sup>™</sup> 7 Pro Real-Time PCR System

#### Kit Components

Component	Product # TM67050 (100 preps)
MDx TaqMan 2X PCR Master Mix	2 x 700 μL
Xylella fastidiosa Primer & Probe Mix	280 μL
Xylella fastidiosa Positive Control	150 μL
Nuclease-Free Water (Negative control)	1.25 mL
Product Insert	1

### **Storage Conditions and Product Stability**

- All kit components should be stored at -20°C upon arrival
- Repeated thawing and freezing (> 2 x) of the Master Mix and Positive Control should be avoided, as this may affect the performance of the assay. If the reagents are to be used only intermittently, they should be frozen in aliquots.

 All kit components can be stored for 2 years after the date of production without showing any reduction in performance.

### **Customer-Supplied Reagents and Equipment**

- Appropriate Real-Time PCR Instrument with FAM and HEX filter channel
- DNA Purification Kit
  - The kit is compatible with all DNA purification kits that yield high quality, inhibitorfree DNA
  - Recommended Purification Kits:
    - Norgen's Plant/Fungi DNA Isolation Kit (Cat. 26200, 26900)
- Disposable powder-free gloves
- Benchtop microcentrifuge
- Micropipettors
- Sterile pipette tips with filters
- PCR tubes
- Vortex mixer
- PCR reaction preparation station (Optional)

#### **Quality Control**

In accordance with Norgen's ISO 9001 and ISO 13485-certified Quality Management System, each lot of Norgen's *Xylella fastidiosa* TaqMan PCR Kit is tested against predetermined specifications to ensure consistent product quality.

### **Warnings and Precautions**

- Norgen's Xylella fastidiosa TaqMan PCR Kit is intended for research purposes only. It is not intended for diagnostic use.
- Follow universal precautions. All specimens should be considered as potentially infectious and handled accordingly.
- Ensure that a suitable lab coat, disposable gloves and protective goggles are worn when handling specimens and kit reagents.
- Use sterile pipette tips with filters. Use proper pipetting techniques and maintain the same pipetting pattern throughout the procedure to ensure optimal and reproducible values.
- As contamination of specimens or reagents can produce erroneous results, it is essential
  to use aseptic techniques. Pipette and handle reagents carefully to avoid mixing of the
  samples.
- Do not use supplies and equipment across the dedicated areas of i) specimen extraction, ii) reaction set-up and iii) amplification/detection. No cross-movement should be allowed between the different areas. Personal protective equipment, such as laboratory coats and disposable gloves, should be area specific.
- Store and extract positive material (specimens, controls and amplicons) separately from all other reagents and add it to the reaction mix in a spatially separated facility.
- Dispose of unused kit reagents and specimens according to local, provincial or federal regulations.
- Do not substitute or mix reagents from different kit lots or from other manufacturers. Do not use components of the kit that have been stored for more than 2 years.
- The presence of PCR inhibitors may cause false negative or invalid results.
- Potential mutations within the target regions of the *Xylella fastidiosa* genome covered by the primers in this kit may result in failure to detect the presence of the pathogen.

- Good laboratory practice is essential for the proper performance of this kit. Ensure that
  the purity of the kit and reactions is maintained at all times, and closely monitor all
  reagents for contamination. Do not use any reagents that appear to be contaminated.
- Ensure that appropriate specimen collection, transport, storage and processing techniques are followed for optimal performance of this test.

### Instructions for Use

### A. Sample Preparation

Purified DNA is the starting material for Norgen's *Xylella fastidiosa* TaqMan PCR Kit. The quality of the DNA template will have a major impact on the performance of the *Xylella fastidiosa* detection test. The user must ensure that the method used for DNA purification is compatible with TaqMan PCR. We recommend the use of Norgen's **Plant/Fungi DNA Isolation Kit (Cat. 26200, 26900).** Norgen's Plant/Fungi DNA Isolation Kit have been fully validated with Norgen's *Xylella fastidiosa* TaqMan PCR Kit.

If using a different spin column based sample preparation procedure that includes ethanol-based wash buffers, a column drying step consisting of centrifugation for 3 minutes at  $20,000 \times g$  (~14,000 RPM), using a new collection tube, is highly recommended prior to the elution of the DNA. This will help to prevent the carry-over of any ethanol into the purified DNA, as ethanol is known to be a strong inhibitor of PCR. **Ensure that any traces of ethanol from the sample preparation steps are eliminated prior to the elution of the DNA**.

## B. TaqMan PCR Assay Preparation

#### Notes:

- Before use, suitable amounts of all TaqMan PCR components should be completely thawed at room temperature, mixed by gentle vortexing or by pipetting, and centrifuged briefly.
- Work quickly on ice.
- The amount of MDx TaqMan 2X PCR Master Mix provided is enough for up to 128 PCR reactions (96 sample PCR, 16 positive control PCR and 16 no template control PCR).
- For every TaqMan PCR run, one reaction containing *Xylella fastidiosa* Positive Control and one reaction as no template control must be included for proper interpretation of results.
- The recommended minimum number of DNA samples tested per TaqMan PCR run is 6.
- To avoid any contamination while preparing the TaqMan PCR assay, follow the order outlined in Tables 1, 2 and 3 below to prepare the Negative Control, Detection Assay and Positive Control:
  - 1. Prepare the PCR Negative Control (Table 1)
  - 2. Prepare the PCR Xylella fastidiosa Assay (Table 2)
  - 3. Prepare the PCR Positive Control (Table 3)
- To further avoid contamination, add the components to the PCR tubes in the order shown in the tables below (ie: 1) Nuclease-free water; 2) MDx TaqMan 2X PCR Master Mix; 3) Primer & Probe Mix; and 4) the Sample DNA or Positive Control).

1. For each TagMan PCR set, prepare one no template control PCR as shown in Table 1 below:

**Table 1. TaqMan PCR Negative Control Preparation** 

PCR Components	Target detection (with MDx TaqMan 2x PCR Master Mix)
Nuclease-Free Water	8 μL
MDx TaqMan 2X PCR Master Mix	10 μL
Xylella fastidiosa Primer & Probe Mix	2 μL
Total Volume	20 μL

2. Prepare the PCR reaction for sample detection as shown in Table 2 below.

Table 2. TaqMan PCR Xylella fastidiosa Assay Preparation

PCR Components	Target detection (with MDx TaqMan 2x PCR Master Mix)
Nuclease-Free Water	5 μL
MDx TaqMan 2X PCR Master Mix	10 μL
Xylella fastidiosa Primer & Probe Mix	2 μL
Sample DNA*	3 µL
Total Volume	20 μL

 $<sup>^*</sup>$  The recommended amount of sample DNA to be used is 3  $\mu L$ . However, a volume between 1 and 5  $\mu L$  of sample DNA may be used as template. Adjust the final volume of the PCR reaction to 20  $\mu L$  using the Nuclease-Free Water provided.

3. For each PCR set, prepare **one** positive control PCR as shown in Table 3 below:

**Table 3. TaqMan PCR Positive Control Preparation** 

PCR Components	Target detection (with MDx TaqMan 2x PCR Master Mix)
MDx TaqMan 2X PCR Master Mix	10 μL
Xylella fastidiosa Primer & Probe Mix	2 μL
Xylella fastidiosa Positive Control (PosC)	8 µL
Total Volume	20 μL

### C. Xylella fastidiosa TaqMan PCR Assay Programming

- 1. Program the thermocycler according to the program shown in Table 4 below.
- 2. Run TaqMan PCR assay.

Table 4. Xylella fastidiosa TaqMan PCR Program


PCR Cycle	Step	Temperature	Duration
Cycle 1	Step 1	95°C	3 min
Cycle 2 (40x)	Step 1	95°C	15 sec
Cycle 2 (40x) Step 2	60°C	30 sec	

# D. Xylella fastidiosa TaqMan PCR Assay Interpretation


Table 5. Interpretation of Assay Results

FAM (Target detection)	HEX (PCR validation)	Result
+	+	Positive
-	+	Negative
-	-	PCR inhibited


For results obtained that are not covered in Table 5, please refer to the Frequently Asked Questions.

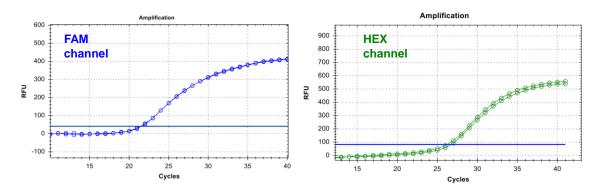

**Figure 1.** Example of TaqMan PCR Positive result. Both PCR signals above the baseline from FAM and HEX channel indicate the successful PCR.

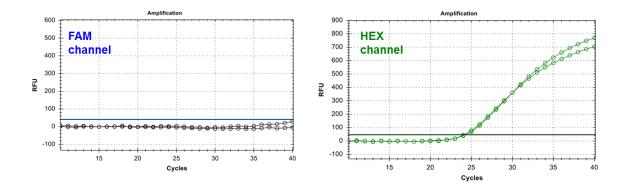

**Figure 2.** Example of TaqMan PCR Negative result. No target DNA was detected in FAM channel but amplification signal from HEX indicates the successful PCR.

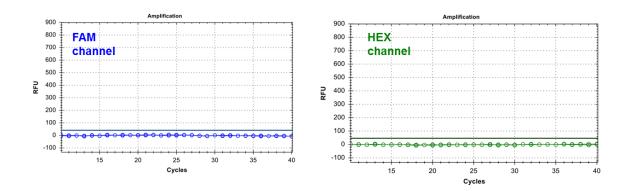

**Figure 3.** Example of TaqMan PCR inhibition result. No signal from both FAM and HEX channel was detected. It is suggested to repeat the sample preparation using recommended kit for DNA purification.

### E. Xylella fastidiosa TaqMan PCR Assay Specificity

The specificity of Norgen's *Xylella fastidiosa* PCR Detection Kit is first and foremost ensured by the selection of the *Xylella fastidiosa*-specific primers, as well as the selection of stringent reaction conditions. The *Xylella fastidiosa* primers were checked for possible homologies to all microorganisms in GenBank published sequences by sequence comparison analysis.

### **Frequently Asked Questions**

- 1. How many samples should be included per PCR run?
  - Norgen's Xylella fastidiosa TaqMan PCR Detection Kit is designed to test 96 samples. For every 6 samples, a non-template control (Nuclease-Free Water) and a Positive Control must be included. It is preferable to collect and test 6 samples at a time.
- 2. How should it be interpreted if no PCR control signal (HEX) is detected while the target specific signal (FAM) is detected in the positive control?
  - Tested samples(s) can be considered positive. It could happen when too much target DNA template was added due to the preferential amplification on the target.
- 3. How should it be interpreted if the target specific signal (FAM) and/or the PCR control signal (HEX) are detected in the negative control?
  - It could happen when there is carryover contamination and PCR inhibition. Repeat the assay using fresh aliquots and clean pipette tips.
- 4 How should it be interpreted if no target signal (FAM) is detected in positive control?
  - It could happen when the positive control was not added. Repeat the assay.

Related Products	Product #
Xylella fastidiosa TaqMan Probe/Primer and Control Set	TM67010
Plant/Fungi DNA Isolation Kit	26200, 26900

### **Technical Support**

Contact our Technical Support Team between the hours of 8:30 and 5:30 (Eastern Standard Time) at (905) 227-8848 or Toll Free at 1-866-667-4362.

Technical support can also be obtained from our website (www.norgenbiotek.com) or through email at techsupport@norgenbiotek.com.

#### **Product Use Restriction**

Norgen's *Xylella fastidiosa* TaqMan PCR Kit is designed for the detection of *Xylella fastidiosa* specific DNA in a real-time PCR based on the use of TaqMan technology. This kit is designed for research use only and not for use in diagnostic procedures.

Norgen's *Xylella fastidiosa* TaqMan PCR Kit is intended for use by professional users such as technicians and biologists experienced and trained in molecular biological techniques including PCR.

Good laboratory practice is essential for the proper performance of this kit. Ensure that the purity of the kit and reactions is maintained at all times, and closely monitor all reagents for contamination. Do not use any reagents that appear to be contaminated.

Ensure that appropriate specimen collection, transport, storage and processing techniques are followed for optimal performance of this test.

The presence of PCR inhibitors may cause false negative or invalid results.

Potential mutations within the target regions of the *Xylella fastidiosa* genome covered by the primers in this kit may result in failure to detect the presence of the pathogen.

The respective user is liable for any and all damages resulting from application of Norgen's *Xylella fastidiosa* TaqMan PCR Kit for use deviating from the intended use as specified in the user manual.

All products sold by Norgen Biotek are subjected to extensive quality control procedures and are warranted to perform as described when used correctly. Any problems should be reported immediately. The kit contents are for laboratory use only, and they must be stored in the laboratory and must not be used for purposes other than intended. The kit contents are unfit for consumption.

TagMan is a registered trademark of Roche Molecular Systems, Inc.

Norgen Biotek Corp.
3430 Schmon Parkway, Thorold, ON Canada L2V 4Y6
Phone: (905) 227-8848
Fax: (905) 227-1061
Toll Free in North America: 1-866-667-4362

©2022 Norgen Biotek Corp.

PITM67050-1